IOT-S300WS7

USER'S MANUAL

LINOVISION

7-in-1 Weather Station User Guide



Tables of Contents

Tables of Contents	3
1 Product Introduction	5
2 Installation	6
2.1 Packing List	6
2.2 Installation	7
2.2.1 Device Interface Introduction	7
2.2.2 Connect with USB Cable	8
2.2.3 M12 Cable	9
2.2.4 Install the device.	11
3 Device's Operating Mode	12
3.1 Configure the device via USB port	13
3.2 Serial debug tool	14
4 Communication Protocols	15
4.1 Modbus-RTU Protocol	16
4.1.1 Modbus-RTU Protocol Message Formats	16
4.1.2 Register Address Definition	17
4.1.3 Modbus-RTU Read	18
4.2 ASCII Protocol	22
4.2.1 Command definition	22
4.2.2 Query Command Format	22
4.2.3 Setting Command Format	23
4.2.4 Command List	23
4.3 SDI-12	30
4.3.1 SDI-12 command and response	30
4.3.2 SDI-12 Read	33
5 Error code	38
5.1 Modbus error code	38

5.2 ASCII error code	38
5.3 SDI-12 error code	38

1 Product Introduction

All-in-One Weather Station is a series of all-in-one compact weather sensors, including, S300WS7 7-in-1 weather sensors. These weather sensors integrate multiple sensors into this compact device, monitoring up to 7 weather parameters: air temperature, air humidity, atmospheric pressure, light intensity, wind speed, wind direction, precipitation. The sensors use ultrasonic to measure wind speed and wind direction, to achieve high-precision data collection, which is easy maintenance. The equipment is designed with industry standards and can work stably in harsh outdoor environments from -40°C to 85°C. The product supports the Modbus-RTU (RS485) and SDI-12 protocols.

Basic parameters			
Product Model	All-in-One Weather Station Series (S300WS7)		
Power Supply	12V~ 24V (0.5W)		
Heating Power Supply	24V (21W)		
Support Protocols	RS485 (MODBUS-RTU) / SDI-12		
IP Rating	IP66		
Working Temperature	-40 °C ~ + 85 °C		
Working Humidity	0 to 100%RH (non-condensing)		

Product Model: S300WS7 (7-in-1)				
Measurement Parameter	Measurement Range	Measurement Accuracy	Resolution	
Air temperature	-40~85°C	±0.1℃	0.01°C	
Air humidity	0~100%RH	±1.5%RH	0.01%RH	
Barometric pressure	300~1250hPa	±50Pa	10 Pa	
Wind speed	0~60 m/s standard range 0~75m/s extended range Up to 80m/s withstand range	±0.3m/s(≤10m/s); ±3% (10m/s ~ 50m/s) ±5% (>50m/s)	0.1m/s	
Direction of the wind	0~360° (@-40°C~60°C)	±3.0°	0.1°	
Light intensity	0~188000 Lux	5% * reading	5Lux	
Rain intensity	0~200mm/h	±10%	0.2mm/0.02mm	

2 Installation


Before the installation, check the packing list and make sure there are no missing parts.

2.1 Packing List

	Parts	Number
•	Linovision All-in-one compact weather sensor	1
•	M12 8-pin communication cable (default length 3-meter hook-up wire)	1
•	USB Type-C cable, for configuring devices	1
•	Pole adapter cross bar	1


2.2 Installation

2.2.1 Device Interface Introduction

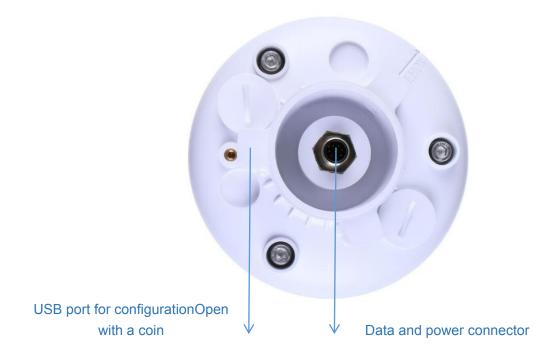

There are two connectors at the bottom of the device.

- USB Type-C interface allows you to connect your computer with a normal USB Type-C cable to the device for configuration.
- The main data interface can be connected to the M12 8-pin cable, supporting multiple bus protocols

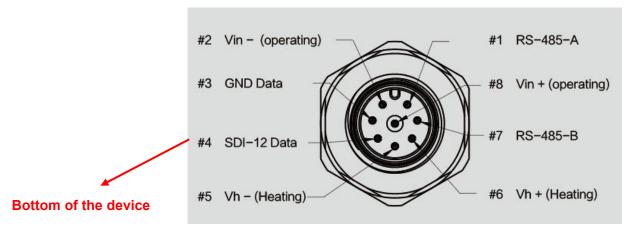


2.2.2 Connect with USB Cable




Note: The white cover (on the side near the label) should be tightened after debugging to prevent water from entering the device!

2.2.3 M12 Cable

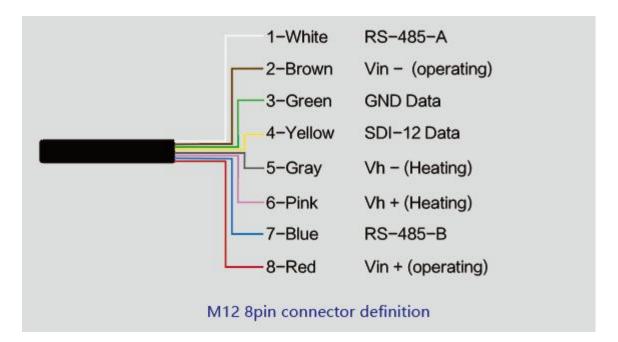

The device adopts an M12 8-pin connector, the different colored pins provide power and data communication (as shown in the above diagram).

When working with the RS-485, you can connect only 4 wires (not using a heating function), and the rest can be individually wrapped with tape to prevent short circuit

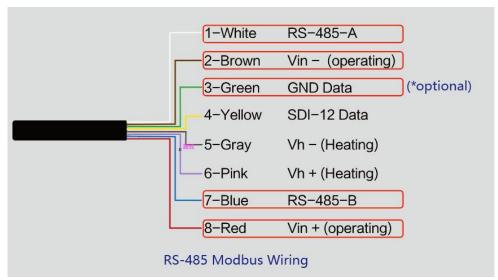

The holes of the cable and the pins of the device connector must be aligned when the cable is plugged in.




Plugin the cable and tighten it clockwise

Note: the cable is aimed at with the bottom before inserting it into the bottom. Otherwise,the pins are skewed may cause the communication is abnormal .




When using the device with a heating function, a separate 24V (24V@1A is recommended) power supply is required. Gray wire #5 is connected to the negative of the power supply, and pink wire #6 is connected to the positive pole of the power supply.

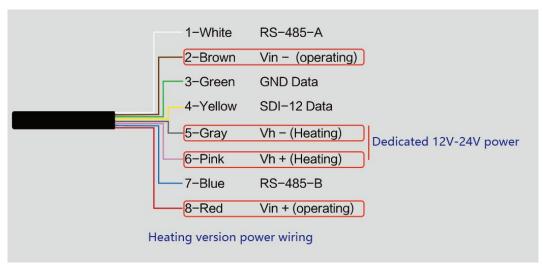

Reminding:

- 1. When the device needs to add power extension cable, if its length is more than 100 meters, it needs to use 24V/2A for power supply (without heating function);
- 2. When the heating function is enabled, the power supply of the heating module should be within 3 meters of the Linovision. The distance between the power supply of the heating module and the device is not more than 5m.

2.2.4 Install the device.

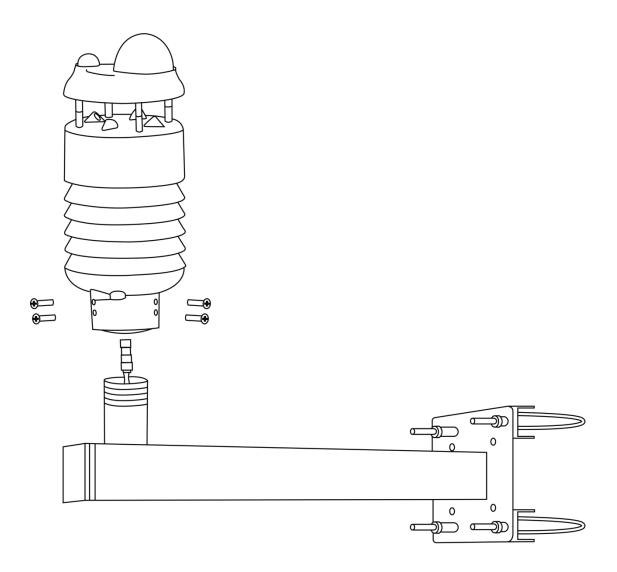

3 Device's Operating Mode

After installation, you can power on the device, configure it and collect data from the device.

The device has two operating modes, configuration mode, and working mode.

	With a USB cable, you can check or configure the device's parameters,	
Configuration Mode	such as device name, version number, and communication protocol	
	configuration. Product firmware can be upgraded in this mode.	
	Connect the devices and data logger with an M12 data and power cable,	
Working Mode	and then the data collected by the device will be sent to the host via	
	different communication protocols.	

3.1 Configure the device via USB port

There is a waterproof round cover at the bottom of the device. Turn it counterclockwise to remove this cover, and you can see a USB Type-C connector and a configuration button.

Connect the device to your computer with a USB Type-C cable. The computer will automatically install the device driver. After the driver is successfully installed, you can see a serial port in the device's manager.



If the driver is not installed automatically, click this link to manually download and install the driver. (The

version is CP210x Windows Drivers)




There are two methods to configure the device:

- Linovision Configuration Tool
- Serial debug tool

3.2 Serial debug tool

The communication settings are as follows:

Select the serial port	You can find port information in your computer's device manager
Baud rate	9600bps, 8 data bits, 1 stop bits, none parity, none flow control.

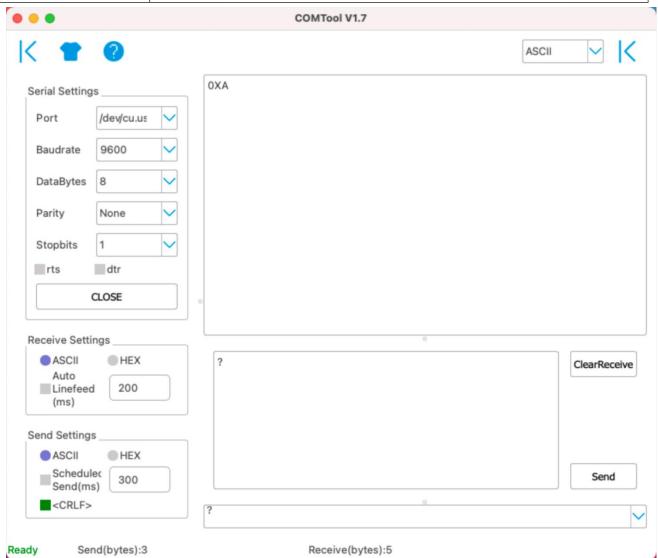

- In the Serial Debug Assistant, select the corresponding COM port.
- Check the "click Enter to start a new line" check box.
- Set the baud rate to 9,600.
- Send ? in the send area.
- If you receive the corresponding 0XA message in the serial receive window, the configuration is successful. If not, please check the COM port and the baud rate.

Please check the detailed ASIIC command in the next chapter.


4 Communication Protocols

The device supports the following communication protocols:

	The Modbus protocol is a common language applied to electronic devices. With this			
	protocol, devices can communicate within their network. It has become a universal			
	industry standard, widely used in data loggers, sensor equipment, and so on. Based on			
Madhua DTU	this protocol, devices produced by different vendors can communicate with each other			
Modbus-RTU for system integration.				
	The Modbus protocol is a master-slave protocol. One node is the host, and the other			
	nodes that use the Modbus protocol to join the communication are the slave. Each slave			
	has a unique address.			
	The ASCII protocol is a query-response or a question-and-answer communicat			
ASCII	protocol in which a host PC uses ASCII characters to send commands to a device and			
	then receives responses from that device.			
OD! 40	Single-bus-based data communication protocol , is an asynchronous serial			
SDI-12	communications protocol for intelligent sensors that monitor environment data.			

4.1 Modbus-RTU Protocol

To start Modbus-RTU communication, the M12 data cable of the device needs to be connected to the RS-485 port of one Data Logger, which powers up the device at a voltage of 12V-24V. The following image is a diagram of the wiring:

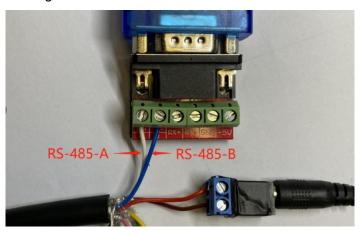

Protocol communication parameters

Data Format	One start bit, 8 Data bits, None parity, one Stop bits.		
Baud Rate	9600bps (default), which can be modified by configuration.		
Default Device Address	\$200W\$7	20	
(Decimal)	S300WS7 20		

4.1.1 Modbus-RTU Protocol Message Formats

Sensor data is stored in the Input Register and is read-only

The device address and the communication baud rate of RS-485 are stored in the Holding Register and can be modified.

Each register is 16bits and takes up 2 bytes.

Read the message from the input register.

The message format from by the host						
Slave address Function code Register address Number of registers CRC check						
1 byte	1 byte	2 bytes (big-endian).	2 Byte (big-endian).	2 bytes		
AA	0x04	RRRR	NNNN	cccc		
Address 0-247	0x04	big endian	big endian	little endian		

The message response from the slave						
Slave address Function code Number of registers First Register data Second register data CRC					CRC check	
1 byte	1 byte	1 byte	2 bytes	2 bytes		2 bytes
AA	0x04	ММ	VV0	VV1		cccc
Address 0-247	0x04	big endian	big endian	big endian		little-endian

Read and write the holding register.

The message format from by the host					
Slave address Function code Register address Number of registers CRC check					
1 byte	1 byte	2 bytes (big-endian).	2 Byte big-endian).	2 bytes	
AA	0x03/0x06	RRRR	NNNN	cccc	
Address 0-247	0x03/06	big endian	big endian	little endian	

The message response from the slave						
Slave address	Function code	Number of	First Register data	Second register		CRC check
		registers		data		
1 byte	1 byte	1 byte	2 bytes	2 bytes		2 bytes
AA	0x03/0x06	MM	VV0	VV1		cccc
Address 0-247	0x03/0x06	big endian	big endian	big endian		little-endian

4.1.2 Register Address Definition


Register	A -1 -1	Name		Number of	Register	N-4-
type	Address	Name	values range	registers	status	Note
	0x0000	Air temperature	-40000~85000	2	R	
	0x0002	Air humidity	0~100000	2	R	
	0x0004	barometric pressure	30000000~125000000	2	R	
	0x0006	Light intensity	0~188000000	2	R	
	0x0008	Minimum wind direction	0~360000	2	R	
	0x000A	Maximum wind direction	0~360000	2	R	
	0x000C	Average wind direction	0~360000	2	R	
Input		R	big endian Data format int32			
register		2	R	Divide the data value by 1000 to get the true measurements		
			0~60000	2	R	
	0x0014	Accumulated rainfall	0~8000000	2	R	
	0x0016	Accumulated rainfall duration	0~200000000	2	R	
	0x0018	Rain intensity	0-200000	2	R	
	0x001A	Maximum rainfall intensity	0-60000	2	R	
	0x001C	Heating Temperature	-40000~85000	2	R	

		The dumping of	0 or 1000((The dumping	_		
	0x001E	state	of state is 1000, the vertical of state is 0)	2	R	
	0x1000	Device address		1	R/W	The default address is 1
	0.1000	Device address		'	TOVV	Can be set to 1 - 247
						The default is 96, which means
						9600.
						It can be set to:
						12=1200
						24=2400
	0x1001	x1001 Baud rate		1	R/W	48=4800
	olding					96=9600
						192=19200
I la ldin a						384=38400
						576=57600
register						1152=115200
	0x2000	Set the		1	R/W	Write 1 to set accumulated
		accumulated				rainfall to 0. Read back 1 to
		rainfall to 0				confirm that the setting is
						finished. Read back 0 indicates
						that the setting failed
	0x2001	Set the accumulated		1	DAM	Write 1 to set accumulated
	0,2001	rainfall duration			R/W	rainfall duration to 0. Read back
						1 to confirm that the setting is
						finished. Read back 0 indicates
						that the setting failed


4.1.3 Modbus-RTU Read

Here is an example of the Modbus Poll tool


(download from https://www.modbustools.com/download.html).

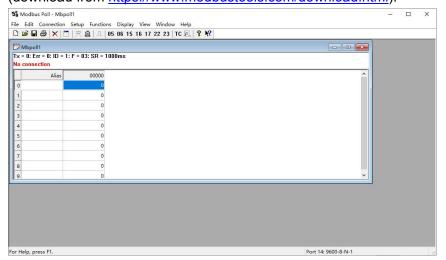


Configuration connection parameters: Baud rate 9600bps, 8 Data bits, None Parity, 1 Stop bits.

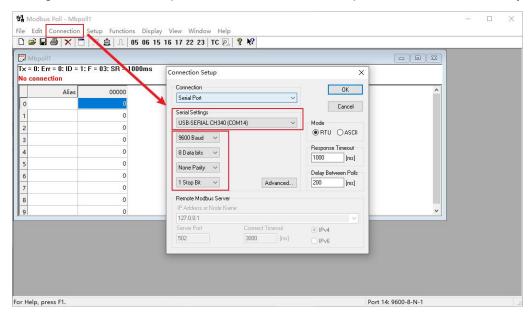


Read the air temperature register 0x0000 to 0x0001, click Setup, and select Read/Write Definition

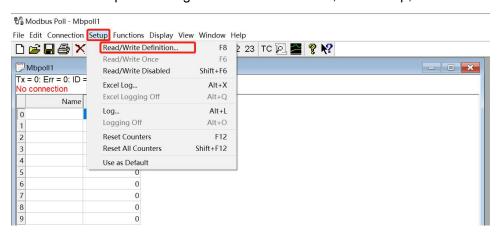

Set the default slave ID(7-in-1 is 20), function code 04, starting address 0, quantity (7-in-1 is 28);

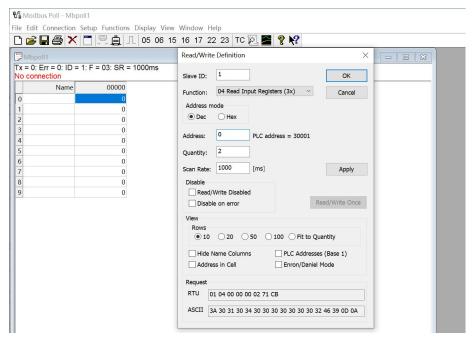

Now the computer reads the sensor data every 1 second, and the measurement (line 0 and line 1) is shown in below picture, after dividing the measurement by 1000, it is the true temperature value, $28300/1000 = 28.3 \,^{\circ}\text{C}$

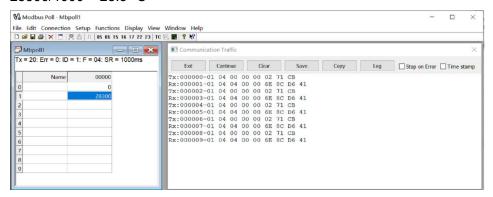

On the right, you can check the raw sent and received data packages.

When the temperature is positive:

- 1. Host sends 01 04 00 00 00 02 71 CB
- 2. Slave responses 01 04 04 00 00 6E 8C D6 41
- Return temperature data 0x00006E8C (Hex), converted to decimal = 28300, get the corresponding air temperature by dividing through 1000, air temperature = 28300/1000 = 28.3 °C

When the temperature is negative:

The temperature needs to be obtained through a complement calculation.

- 1. Host sends 01 04 00 00 00 02 71 CB
- 2. Slave responses 01 04 04 FF FF FC 18 D6 41
- 3. Returned temperature data FFFFC18H (Hex complement).
- 4. The original code is (FF FF FC 18-1 = FF FF FC 17) = 80 00 03 E8(Hex) = -1000 (Decimal).
- 5. Then the temperature measurement is $-1000/1000 = -1^{\circ}$

S300WS7 decode:

Read register: 0x0000~0x001F

Send command: 14 04 00 00 00 20 F3 17

Return: 14 04 40 00 00 70 80 (Temperature) 00 00 95 10 (Humidity) 06 07 94 40 (Air pressure) 00 00 00 00 (Light) 00 00 00 00 (Min wind direction) 00 00 00 (Max wind direction) 00 00 00 00 (Avg wind direction) 00 00 00 00 (Min wind speed) 00 00 00 (Max wind speed) 00 00 00 00 (Avg wind speed) 00 00 00 00 (Accumulated rainfall) 00 00 00 00 (Accumulated rainfall duration) 00 00 00 (Rain intensity) 00 00 00 00 (Maximum rainfall intensity) 00 00 6A 7C (Heating Temperature) 00 00 00 00 (The dumping of state) 99 09 (Check code)

4.2 ASCII Protocol

4.2.1 Command definition

Α	Device address, 0 by default
XA	Starter, fixed value
;	The separator used to distinguish multiple commands
	A command, represented by different strings
?	A query term used to query values
=	Assignment, which is used to set the value
v	The argument, the specific value of the parameter is set
m	Sensor measurement
&	Sensor measurements combine character for getting or setting multiple
α	measurement parameters
<cr><lf></lf></cr>	Response terminator


Terms Explanation

Command	Represented by different strings, such as BD for Baud rate and CP for		
Command	communication protocol		
	A Data List contains multiple sensor measurement types, represented by an		
Data List	abbreviation of G0.		
Data List	For example, G0 contains several test types:		
	AT;AH;AP;LX;DN;DM;DA;SN;SM;SA;RA;RD;RI;RP;HT;TILT		

4.2.2 Query Command Format

Commands come in two formats:

1. A command without = refers to the basic query method.



Example: ?<CR><LF> indicates query the device's address

2. A command with = refers to a query with an argument



Example: 0XA;BD=?<CR><LF> indicates query the device's baud rate

4.2.3 Setting Command Format

Set a specified parameter, such as setting a baud rate.



Example: 0XA;BD=96<CR><LF> indicates query the device's baud rate

4.2.4 Command List

Device info queries and related commands settings

Query De	vice address	?				
	Send	? <cr><lf></lf></cr>	? <cr><lf></lf></cr>			
Query	Response	0XA <cr><lf></lf></cr>	0XA <cr><lf></lf></cr>			
	Description	The default respons	e address is 0			
Query ba	ud rate	BD				
	Send	0XA; BD=? <cr><l< td=""><td>:></td></l<></cr>	:>			
Query	Response	0XA; BD=96 <cr><</cr>	F>			
	Description	The baud rate for de	vice 0 is 9,600			
	Send	0XA; BD=[bd] <cr></cr>	:LF>			
	Response	0XA; BD=[bd] <cr></cr>	tLF>			
Setting		Return the Baud rat	e of device 0 is [bd], it could be 96 for 9600; 192 for 19200, 384 for 38400; 576 for			
	Description	57600; and 1152 for	115200.			
		For example, the re	For example, the return value 0XA;BD=96 represents the successful setting of a Baud rate of 9,600			
Communication protocol		CP				
	Send	0XA; CP=? <cr><l< td=""><td></td></l<></cr>				
	Response	0XA; CP=[cp] <cr></cr>	0XA; CP=[cp] <cr><lf></lf></cr>			
		[cp] Represents the code of the communication protocol, the device supports multiple communication				
		protocols.				
Query		1	SDI-12			
440.7	Description	2	RS-485 Modbus-RTU			
		3	RS-485 ASCII			
		Response 0XA;CP=3 <cr><lf> means that the data communication protocol of device 0 is Modb</lf></cr>				
		protocol based on the RS-485 bus				
RS-485 address MBAD						
	Send	0XA; MBAD=? <cr></cr>	<lf></lf>			
Query	Response	0XA; MBAD=1 <cr></cr>	<lf></lf>			
	Description	The RS-485 addres	The RS-485 address of device 0 is 1 (decimal)			
Setting	Send	0XA; MBAD=2 <cr><lf></lf></cr>				

	Response	0XA; MBAD=2 <cr><lf></lf></cr>				
	Description	Set the address of device 0 to 2 (decimal)				
RS	3-485 baud rate	MBBD				
	Send	0XA; MBBD=? <cr><lf></lf></cr>				
Query	Response	0XA; MBBD=96 <cr><lf></lf></cr>				
	Description	The RS-485 communication baud rate for device 0 is 9,600				
	Send	0XA; MBBD=[bd] <cr><lf></lf></cr>				
	Response	0XA; MBBD=[bd] <cr><lf></lf></cr>				
Setting		Return device 0's RS-485 communication baud rate is [bd]: it can be 96 for 9600, 192 for 19200, 384 for				
Setting	Description	38400, 576 for 57600, and 1152	for 115200.			
	Description	For example, the return value is 0	0XA;MBBD=96 represents the successful setting of the	e baud rate of		
		9,600				
D	evice version	VE				
	Send	0XA; VE=? <cr><lf></lf></cr>				
Query	Response	0XA; VE=HW-1.0&SW-2.0&S1-2	.2 <cr><lf></lf></cr>			
	Description	Device hardware(HW) is v1.0, the	e software firmware(SW) is v2.0, and the #1 driver boa	ard firmware is v2.2		
Devi	ce serial number	S/N				
	Send	0XA; S/N=? <cr><lf></lf></cr>				
Query	Response	0XA; S/N=1019906922012011<0	CR> <lf></lf>			
	Description	S/N represents the serial number	r of the device			
Pr	oduction date	MD				
	Send	0XA; MD=? <cr><lf></lf></cr>				
Query	Response	0XA; MD=20201027 <cr><lf></lf></cr>				
	Description	The production date of the return device is October 27, 2020, 20201027				
Rest	ore configuration	RESTORE				
	Send	0XA; RESTORE=1 <cr><lf></lf></cr>				
Setting	Response	0XA; RESTORE=1 <cr><lf></lf></cr>				
	Description	Return 0XA; RESTORE=1 means the setting is successful and return 0XA means the setting fails.				
Elec	tronic Compass	cc				
	Send	0XA;CC=? <cr><lf></lf></cr>				
	Response	0XA;CC=[cc] <cr><lf></lf></cr>				
Query		[cc] Electronic Compass offset st				
	Description	Y	Enable Electronic Compass			
		N	Disable Electronic Compass			
		C Enable Geomagnetic compensation				
	Send	0XA;CC=Y <cr><lf></lf></cr>				
	Response	0XA;CC=Y <cr><lf></lf></cr>				
	Description	Enable Electronic Compass				
Setting	Send	0XA;CC=N <cr><lf></lf></cr>				
	Response	0XA;CC=N <cr><lf></lf></cr>				
	Description	Disable Electronic Compass				
	Send	0XA;CC=C <cr><lf></lf></cr>				
	Response	0XA;CC=C <cr><lf></lf></cr>				

	5	Enable Geomagnetic compensation, it will start the 30s compensation process, during this time, the
	Description	device should be placed horizontally, and rotate evenly along the Z-axis for 1-2 rounds.
	Tilt Detect	TD
	Send	0XA;TD=? <cr><lf></lf></cr>
0	Response	0XA;TD=Y/N <cr><lf></lf></cr>
Query	5	Y: Enable tilt detection function
	Description	N: Disable tile detection function
	Send	0XA;TD=Y <cr><lf></lf></cr>
	Response	0XA;TD=Y <cr><lf></lf></cr>
	December	Set to enable tilt detection function: TILT=0 means the device is placed vertically, TILT=1 means the
Setting	Description	device is placed not placed upright.
	Send	0XA;TD=N <cr><lf></lf></cr>
	Response	0XA;TD=N <cr><lf></lf></cr>
	Description	Disable tile detection function: the TILT always equals 0 when the device is placed at any position.
	Heating	нс
	Send	0XA; HC =? <cr><lf></lf></cr>
0	Response	0XA; HC =Y/N <cr><lf></lf></cr>
Query		Y: enable heating function
	Description	N: disable heating function
Send		0XA;HC=Y <cr><lf></lf></cr>
	Response	0XA;HC=Y <cr><lf></lf></cr>
		Turn on the heating function of the device;
		When the air temperature is between [5 $^{\circ}\mathrm{C}$ and -25 $^{\circ}\mathrm{C}$], the device begins to heat, and the
		temperature of the heating plate is the highest, up to $40^{\circ}\mathrm{C}$
Setting	Description	When the air temperature is higher than 5 ° C, the device stops to heat;
Setting		(Note: If the temperature is lower than -25 $^{\circ}$ C ,the heating module cannot raise the
		temperature of the device above 0 ° C, it may freeze, which will affect the detection of
		wind speed and direction)
	Send	0XA;HC=N <cr><lf></lf></cr>
	Response	0XA;HC=N <cr><lf></lf></cr>
	Description	Set to enable heating function.

Command to read sensor data.

For quick reading of all measurements, G0 is the command.

Read all m	easurements	G0
	Send	0XA; G0? <cr><lf></lf></cr>
Ouem	y Response	0XA;AT=23.6;AH=56.4;AP=100819.1;LX=93.0;DN=0.0;DM=0.0;DA=0.0;SN=0.0;SM=0.0;SA=0.0;RA=1.4
Query		;RD=60.0;RI=0.0;RP=0.0;HT=-38.4;TILT=0.0 <cr><lf></lf></cr>
Description		Returns the value of all measurement parameters

Group	Measurement	Name	Unit		
Name	Weasurement	Name	Onit		
G0	Contains all combinations of measurement parameters				

AT	Air temperature	°C (default), °F
AH	Air humidity	%RH
AP	Barometric pressure	Pa (default), hPa, bar, mmHg, inHg
LX	Light intensity	Lux
DN	Minimum wind direction	deg
Dm	Maximum wind direction	deg
DA	Average wind direction	deg
SN	Minimum wind speed	m/s (default), km/h, mph, knots
SM	Maximum wind speed	m/s (default), km/h, mph, knots
SA	Average wind speed	m/s (default), km/h, mph, knots
RA	Accumulated rainfall	mm (default), in
RD	Duration of rainfall	s
RI	Rainfall intensity	mm/h (default), in/h
Rp	Maximum rainfall intensity	mm/h (default), in/h
НТ	Heating temperature	°C
TILT	Fall detection	

Modify the Properties of Measurement Parameters

Properties represent some characteristics of the measured data, such as the unit of output temperature and the interval between data updates.

Tomporature on	and the interval between data updates. Temperature and Humidity Data				
Update Interval		IB			
opaato intol tal	Send	0XA:IB=? <cr><lf></lf></cr>			
Query	Response	0XA:IB=1 <cr><lf></lf></cr>			
Query	•				
	Description	The default data updates every 1 second			
	Send	0XA;IB=2 <cr><lf></lf></cr>			
Setting	Response	0XA;IB=2 <cr><lf></lf></cr>			
	Description	Set the data update interval to 2 seconds, you can choose a value between 1 to 3600 seconds.			
Air Temperature	Unit	UT			
	Send	0XA; UT=? <cr><lf></lf></cr>			
Query	Return	0XA; UT=C <cr><lf></lf></cr>			
	Description	The temperature unit is Celsius			
	Send	0XA; UT=F <cr><lf></lf></cr>			
0-4	Response	0XA; UT=F <cr><lf></lf></cr>			
Set up	Description	Set the air temperature unit to Fahrenheit.			
		C=°C, F=°F			
Barometric Pres	ssure Unit	UP			
	Send	0XA; UP=? <cr><lf></lf></cr>			
Query	Response	0XA; UP=P <cr><lf></lf></cr>			
	Description	The unit is Pa.			
	Send	0XA; UP=H <cr><lf></lf></cr>			
Catum	Response	0XA; UP=H <cr><lf></lf></cr>			
Set up	D	Set the unit to hPa.			
	Description	P = Pa, H = hPa, B = bar, M = mmHg, I=inHg			

Wind Speed & Direction Data Update Interval				
		lW		
	Send	0XA; IW=? <cr><lf></lf></cr>		
Query	Response	0XA; IW=1 <cr><lf></lf></cr>		
	Description	The default data updates every 1 second.		
Send		0XA; IW=2 <cr><lf></lf></cr>		
Set up	Response	0XA; IW=2 <cr><lf></lf></cr>		
	Description	Set the data update interval to 2 seconds, you can choose a value between 1 to 3600 seconds.		
Wind speed & d	irection average	Aug.		
time window		AW		
	Send	0XA; AW=? <cr><lf></lf></cr>		
Query	Response	0XA; AW=5 <cr><lf></lf></cr>		
Query	Description	The default average update interval for wind speed & direction data is 5 seconds.		
	Description	The device collects wind speed & direction in 5s intervals and then averages the value.		
	Send	0XA; AW=10 <cr><lf></lf></cr>		
Setting	Response	0XA; AW=10 <cr><lf></lf></cr>		
	Description	Set the data update interval to 10 seconds, you can choose a value between 1 to 3600 seconds		
Wind Speed Un	it	us		
	Send	0XA; US=? <cr><lf></lf></cr>		
Query	Response	0XA; US=M <cr><lf></lf></cr>		
	Description	The default wind speed unit is m/s		
	Send	0XA; US=K <cr><lf></lf></cr>		
0-44	Response	0XA; US=K <cr><lf></lf></cr>		
Setting	Description	Set unit to km/h		
	Description	M = m/s, K = km/h, S = mph, N = knots		
The wind direct	ion offset	DO		
correction value)			
	Send	0XA;DO=? <cr><lf></lf></cr>		
Query	Response	0XA; DO=0 <cr><lf></lf></cr>		
	Description	The default correction angle for the wind direction is 0.		
	Send	0XA; DO=1 <cr><lf></lf></cr>		
	Response	0XA; DO=1 <cr><lf></lf></cr>		
Setting		Set the wind direction offset to +10°, if the current wind direction is 280°, the corrected wind direction is		
	Description	290 degrees.		
		The wind correction range is -180° to 180°		
Rainfall Data Update Interval		IR		
	Send	0XA;IR=? <cr><lf></lf></cr>		
Query	Response	0XA;IR=10 <cr><lf></lf></cr>		
	Description	The default rain data update interval is 10 seconds.		
	Send	0XA;IR=60 <cr><lf></lf></cr>		
Sotting	Response	0XA;IR=60 <cr><lf></lf></cr>		
Setting	Description	Set the data update interval to 60seconds.		
	Describitori	The interval range is 10 to 3600 seconds.		

Rainfall Unit		UR			
Send		0XA; UR=? <cr><lf></lf></cr>			
Query	Response	0XA; UR=M <cr><lf></lf></cr>			
	Description	The default rainfall unit is mm			
	Send	0XA; UR=I <cr><lf></lf></cr>			
Catting	Response	0XA; UR=I <cr><lf></lf></cr>			
Setting	Description	Set the units of rainfall to inches			
	Description	M = mm, I = inch.			
Rainfall Counte	r Reset Mode	CR			
	Send	0XA; CR=? <cr><lf></lf></cr>			
Query	Response	DXA; CR=M <cr><lf></lf></cr>			
	Description	Rain counter reset mode is by manual M			
	Send	0XA; CR=L <cr><lf></lf></cr>			
	Response	0XA; CR=L <cr><lf></lf></cr>			
		Set the counter reset mode to overflow reset, and you can select the modes as:			
Setting		M: Manual reset, reset immediately after sending the reset command (the reset command is available			
Setting	Description	under all three communication protocols, as detailed in the different protocol sections).			
	Description	A: Post-read reset (accumulated rainfall and accumulated rainfall time are performed separately after			
		reading reset)			
		L: Overflow reset			
Accumulated ra	infall overflow	AL			
	Send	0XA; AL=? <cr><lf></lf></cr>			
	Response	0XA; AL=80000 <cr><lf></lf></cr>			
Query	Description	The default accumulated rainfall overflow value is 80000, which is measured in the current rainfall unit.			
		This overflow value takes effect only if the CR rainfall counter reset mode is set to L overflow reset.			
	Send	0XA; AL=1000 <cr><lf></lf></cr>			
0-44	Response	0XA; AL=1000 <cr><lf></lf></cr>			
Setting	Description	When the rainfall is set to 1000 (current unit), the accumulated rainfall will be reset to 0.			
	Description	The overflow value range is 10-80000 (current unit).			
Accumulated ra	infall duration	DL			
overflow value	Send	0XA; DL=? <cr><lf></lf></cr>			
	Response	0XA; DL=2000000 <cr><lf></lf></cr>			
Query	Response	The default rainfall duration overflow value is 2,000,000, the unit is second.			
	Description	This overflow value will only take effect when the CR rainfall counter reset mode is L overflow reset.			
	Send	0XA; DL=3600 <cr><lf></lf></cr>			
	Response	0XA; DL=3600 <cr><lf> 0XA; DL=3600<cr><lf></lf></cr></lf></cr>			
Setting	response	Set the rainfall duration overflow value to 3600 seconds.			
	Description	It ranges between 100 – 2000000 seconds.			
Clear the accumulated rainfall		CRA			
Olear tile acculi					
Setting	Send	0XA; CRA=1 <cr><lf></lf></cr>			
	Response	0XA; CRA=1 <cr><lf></lf></cr>			

	Description	Clear the accumulated rainfall.	
Clear accumulated rainfall Duration		CRD	
Send		0XA; CRD=1 <cr><lf></lf></cr>	
Setting	Response	0XA; CRD=1 <cr><lf></lf></cr>	
Description		Clear the accumulated rainfall duration.	
Interpretation	Accumulated rainfal	Once the device is powered ,the accumulated value will be calculated and saved. When the accumulated value reaches 80,000 mm, it will be automatically cleared and enter the recalculation stage (it will still saved after power off).	
	Accumulated rainfall duration	Once the device is powered ,the accumulated value will be calculated and saved. When the accumulated value reaches 2000000s, it will be automatically cleared and enter the recalculation stage (it will still be saved after power off).	
	Rainfall intensity (hourly rainfall)	The accumulated rainfall in the past hour, during which the accumulated value is updated every 10s until the accumulated time reaches 1 hour	
	Maximum rainfall intensity	Maximum rainfall per minute in the past hour *60 minutes	


4.3 **SDI-12**

SDI-12 communication adopts three wires, two of which are sensor power supply wires and the other is SDI-12 signal wire.

Each sensor on the SDI-12 bus has a unique address, which can be set to '0', '1' \sim '9', 'A' \sim 'Z', 'A' \sim 'Z'. The SDI-12 address of the Linovision defaults to '0'. The instructions supported by this sensor are shown in the next chapter, where each instruction conforms to the SDI-12 v1.4.

The sensor is powered by a DC power supply of 3.6~16V. After the sensor is powered on, it will go into sleep mode immediately and wait for the data acquisition equipment to give instructions. SDI-12 uses baud rate 9600bps, 1 start bit (high level), 7 data bits (high 0 and low 1, anti-logic), 1 even parity bit, and 1 stop bit.

The sequence of each byte sent is shown in the following figure:



4.3.1 SDI-12 command and response

Command format

- Start with device address 'a', it is '0'in the following sample.
- End with '!'as a terminator
- The response command end with the <CR><LF>

Query the device address	?!
Send	?!
Response	0 <cr><lf></lf></cr>
Description	The sensor at address '0' responded to the query
Query the device	0!
status	
Send	0!
Response	0 <cr><lf></lf></cr>
Description	Address '0' of device online
Modify device	0Ab!
address	
Send	0A1!
Response	1 <cr><lf></lf></cr>
Description	Device address 0 is changed to 1. The address range is 0-9 \ A-Z \ a-z.


Start Measurement	OM!		
Send	ОМ!		
D	Immediately respon	nse: 00024 <cr><lf></lf></cr>	
Response	After 2s, the response device's address, means finishing the measurement.: 0 <cr><lf></lf></cr>		
	This command is	to start THPL measurement, in order: air temperature	e, air humidity, atmospheric
	pressure, illuminance, but the sensor will not reply to the measurement data immediately after receiving		
	this command, but the time required to reply the measurement data and the number of measurements.		
	To obtain measurement data, you must wait until the measurement is completed, and then use the send		
	data command "0D0!" to obtain it.		
	After using this command, the sensor will enter a sleep mode after the measurement to save power		
Description	consumption. After using "continuous measurement command 0R0!0R9!", it will exit the low power		
Description	consumption state.		
	The response form	at is defined as follows:	
	atttn <cr><lf></lf></cr>		
	а	Device address:0	
	ttt	The time expense to measure data, the unit is	
		seconds.	
	n	The number of measurements	
Extended	0M1!0M9!		
Measurement			
Send	0Mn! (n ranges 0~	9)	
Decrees	Immediately response: 00024 <cr><lf></lf></cr>		
Response	After 2s, the response device's address, means finishing the measurement.: 0 <cr><lf></lf></cr>		
	0M1!: Start Wind m	neasurement: minimum wind direction, maximum wind di	rection, average wind
	direction, minimum wind speed, maximum wind speed, average wind speed.		
	0M2!: Start Rain measurement: accumulated rainfall, accumulated rainfall time, rainfall intensity,		
	maximum rainfall intensity.		
	UM9!: Start other m	neasurements: heating temperature, tilt status.	
Description	0M4!0M8!: reserv	her	
Bescription	OWIOWIO:: Teserv	rod.	
	After using this cor	mmand, the sensor will enter a sleep mode after the me	easurement to save power
	consumption. After using "continuous measurement command 0R0!0R9!", it will exit the low power		
	consumption state.		
	For the definition of	f reply, please refer to "Start measurement command 0M	1!"
Read	0D0!0D9!		
measurement			
value			
Send	0D0!		

_				
Response	0+27.65+65.81+100000+5000 <cr><lf></lf></cr>			
	This command is used to obtain a set of measurement data in the sensor. The sensor responds with the			
	measurement data. If all the desired measurement data is not returned in 0D0!, you can continue to			
	send 0D1!, 0D2!, etc., until all the measurement data is received.			
	The response form	at is defined as follows:		
	a <values><cr><lf></lf></cr></values>			
	а	Device address:0		
	<values></values>	This the real measurement value.		
Description		pd.d		
		p is the polarity symbol.		
		the first d is the number before the decimal point.		
		the second d is the data after the decimal point.		
		Note that the decimal point is not necessary.		
		In this example, "+27.65" is the first measurement data, "+65.81" is the		
		second measurement data, "+100000" is the third measurement data, and		
		"+5000" is the fourth measurement data.		
Continuous	0R0!0R9!			
measurement				
command				
Send	ORO!			
Response	0+27.65+65.81+100000+5000 <cr><lf></lf></cr>			
	This is different from "start measurement command 0M!", the measurement value can be returned			
	directly. Each "continuous measurement command" is an independent measurement process, for			
	example, 0R0! and 0R1! are not required before 0R2!.			
	0R0!: Start continuous THPL measurement: air temperature, air humidity, atmospheric pressure, light			
	intensity.			
	0R1!: Start Wind continuous measurement: minimum wind direction, maximum wind direction, average			
Description	wind direction, minimum wind speed, maximum wind speed, average wind speed.			
	0R2!: Start Rain measurement: accumulated rainfall, accumulated rainfall time, rainfall intensity,			
	maximum rainfall intensity.			
	0R9!: Start another Continuous measurement: heating temperature, dumping status.			
	0R4!0R8!: reserved.			
		n a low-power working state before, after using this command, the sensor will exit	t the	
_	low-power working state.			
Start Measurement	aMC!,aMC1!aMC9!,aRC0!aRC9!			
with CRC				
Send	ORCO!			
Response	0+26.52+67.73+100280+35JKy			
	To enhance the error detection capability of the SDI-12 protocol, "start measurement command 0M!",			
	"extended measurement command 0M1!0M9!" and "continuous measurement command 0R0!0R9!"			
Description	can add 16-bit cyclic redundancy check. Add the character C after the command character M or R of			
	these commands to form a new command: aMC!,aMC1!aMC9!,aRC0!aRC9!.			
	For the calculation of CRC-16, please refer to the SDI-12 protocol v1.4 document.			
Clear accumulated	0XCRA!			

rainfall command			
Send	0XCRA!		
Response	01 <cr><lf></lf></cr>		
	aN <cr><lf></lf></cr>		
Description	а	Device address:0	
Description	N	Clear success: 1	
		Clear failed: 0	
Clear accumulated	0XCRD!		
rainfall duration			
Send	0XCRD!		
Response	01 <cr><lf></lf></cr>		
	aN <cr><lf></lf></cr>		
Description	а	Device address:0	
Description	N	Clear success: 1	
		Clear failed: 0	

4.3.2 SDI-12 Read

Wiring the SDI-12

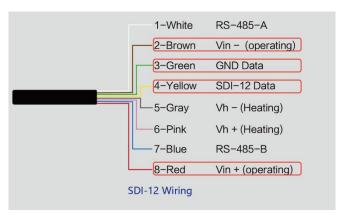

Use USB to SDI-12 debugger to communicate with the device



The communication settings:


Format	1 start bits, 7 data bits, Even parity, 1 stop bits
Baud rate	1200bps

Device address 0x00

Connect the green wire (GND Data) and yellow wire (SDI-12 Data) to the **USB to SDI-12** debugger. And connect the red wire (Vin+ power positive) and brown wire (Vin- power ground) to the 12V power supply.

Download the serial port debugging assistant: https://github.com/Neutree/COMTool, and then open the serial port debugging tool.


- Choose the correct port number
- Set the baud rate to the baud rate of the USB to SDI-12 debugger (note that it is not the baud rate of the SDI-12 protocol)
- Check the "CRLF"
- Click to open the serial port.
- Send the query device address command "?!", if you can see the response "0", it means the connection is OK.

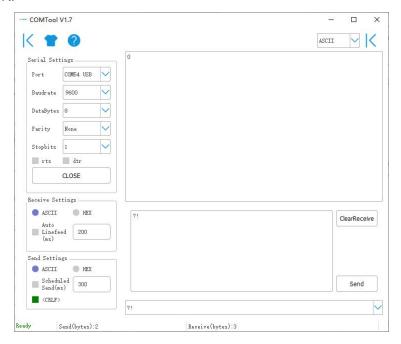


Start Measurement

Read air temperature, air humidity, barometric pressure, light intensity


Send the "start measurement command 0M!", the sensor first responds with "00024", which means that the "0M!" command takes 2 seconds to measure and returns 4 measured values. After 2 seconds, the sensor responds with its own address "0", indicating that the measurement has been completed.

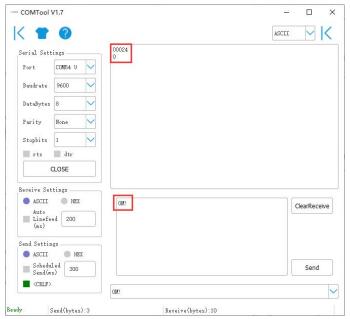


Then send "Read measurement value command 0D0!" to get the 4 measured values of this measurement, which are air temperature $+27.01^{\circ}$ C, air humidity 64.74%, barometric pressure 100720Pa, and light intensity 10Lux.

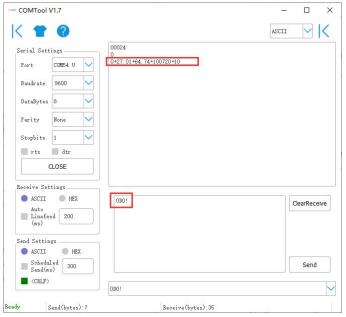


Use extended measurement command 0M1! to read minimum wind direction, maximum wind direction, average wind direction, minimum wind speed, maximum wind speed, average wind speed. The device responds with "00056", which means that the "0M1!" command takes 5 seconds to measure and returns 6 measured values. After 5 seconds, the device responds with its own address "0", indicating that the measurement has been completed.

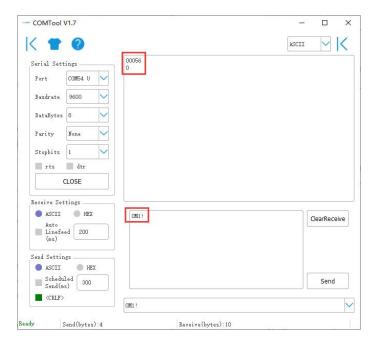

Then send "Read measurement value command 0D0!" to get the 6 measured values of this measurement, which are minimum wind direction 345.9 degrees, maximum wind direction 347.5 degrees, average wind direction 346.3 degrees, minimum wind speed 2.8m/s, and maximum wind speed 2.8m. /s, average wind speed 2.8m/s.

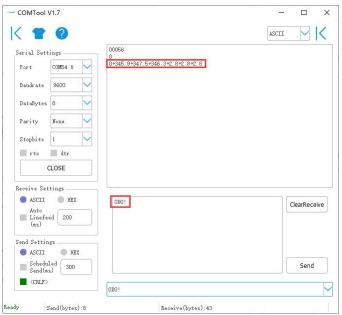

Then send "continuous measurement command 0R2!, the device returns 4 measured values: cumulative rainfall 1.2mm, cumulative rainfall duration 20 seconds, rainfall intensity 1.2mm/h, maximum rainfall intensity 72.0mm/h.

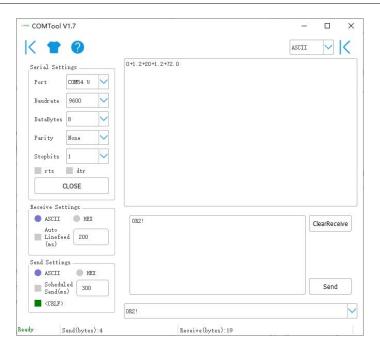

5 Error code

5.1 Modbus error code

Error code	Description	Response instance
0x01	Device do not response	01 84 01 82 C0
0x04	Sensor probe exception	01 84 04 42 C3

5.2 ASCII error code

Error code	Description	Response instance
0	Command do not exist	0XA;=#0
1	Device do not response	0XA;AT=#1
3	The command length exceeds the limit, it	0XA;=#3
	needs to be reduced	
4	Sensor probe exception	0XA;AT=#4

5.3 SDI-12 error code

Error code	Description	Response instance
2001001	Device do not response	0+2001001+2001001+2001001+2001001 <cr><lf></lf></cr>
2001004	Sensor probe exception	0+2001004+2001004+2001004+2001004 <cr><lf></lf></cr>